


# Auxiliary Cart - Camera Cart

## User Manual

MAN-0573 Revision D

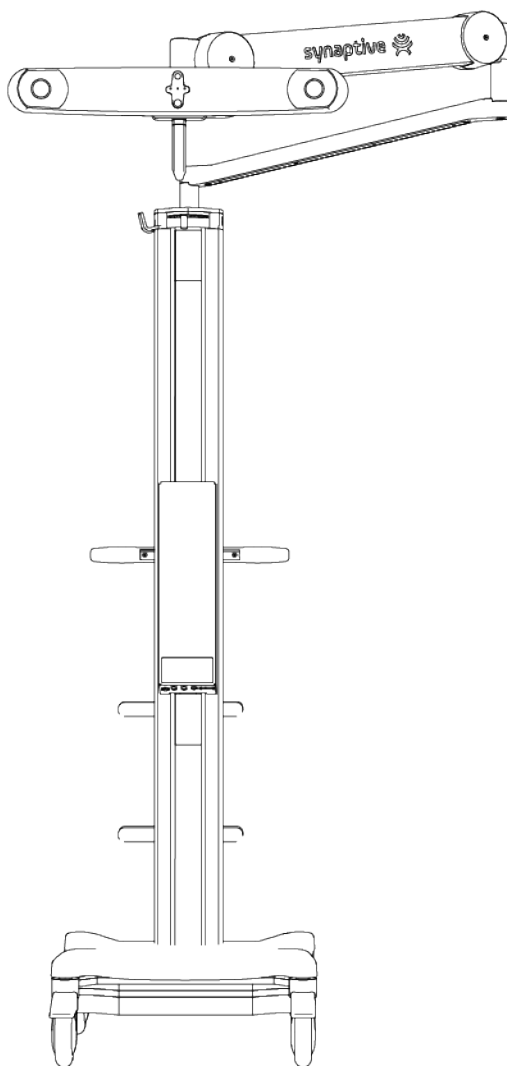

# User Manual

Synaptive™ Auxiliary Cart - Camera Cart

SYN-0621



MAN-0573 – Revision D issued on May 27, 2021.

© 2021 Synaptive Medical

All rights reserved. This document may only be used under license. No part of the document may be reproduced, transcribed, transmitted, distributed, modified, merged or translated into any language in any form by any means – graphic, electronic, or mechanical, including but not limited to photocopying, recording, taping or information storage and retrieval systems – without the prior written consent of Synaptive Medical.

Synaptive, the Synaptive logo, BrightMatter, ClearCanvas, ImageDrive, Solais, Modus Plan, Modus Nav, Modus V, and Evry are trademarks of Synaptive Medical Inc. or its subsidiaries and are protected by law in Canada, the United States, and internationally. All other product and company names mentioned may be trademarks or trade names of their respective owners. Patents pending.

These instructions for use are also available in electronic form at [www.synaptivemedical.com/eIFU](http://www.synaptivemedical.com/eIFU). The electronic instructions for use may be viewed on any device that can access the internet and display PDF files. Access to the electronic instructions for use requires a password; to obtain the password, contact Synaptive Customer Service.

Auxiliary Cart fulfills all the relevant provisions in Regulation (EU) 2017/745 of the European Parliament and of the Council. Based on this regulation, the CE mark is hereby affixed:



**Australian Sponsor:**

KD&A Pty Ltd  
286 Flinders Street  
Adelaide  
South Australia, 5000



Synaptive Medical Inc.  
555 Richmond Street West, Suite 800  
Toronto Ontario M5V 3B1 Canada  
1-844-462-7246  
[www.synaptivemedical.com](http://www.synaptivemedical.com)








EU Authorized Representative:  
Medical Device Safety Service (MDSS)  
Schiffgraben 41  
30175 Hannover, Germany

# Table of Contents




1.0 Product and Safety Symbols .....	4
2.0 Warnings and Precautions .....	6
3.0 Incident Reporting .....	8
4.0 Intended Use Environment .....	8
5.0 Synaptive Customer Service Information .....	8
6.0 About the Auxiliary Cart - Camera Cart .....	8
7.0 About the Tracking Camera .....	9
7.1 Using the Tracking Camera Positioning Laser .....	9
7.2 Positioning Laser Battery .....	10
8.0 Using the Tracking Camera Arm .....	10
9.0 Cart Connections .....	12
10.0 Cleaning .....	12
11.0 Troubleshooting Problems .....	13
12.0 Recommended Environmental Conditions .....	13
13.0 Disposal .....	13
14.0 System Classification and Specifications .....	14
15.0 Essential Performance .....	14
16.0 Specifications .....	14
16.1 Cable Specifications .....	14
16.2 Tracking Camera Laser Specifications and Standards .....	14
17.0 Certifications .....	15
18.0 Electromagnetic Environment Information .....	15

## 1.0 Product and Safety Symbols




**Table 1 ISO 7000 - Graphical symbols for use on equipment - Registered symbols and ISO 15223-1 - Medical devices - Symbols to be used with medical device labels, labeling and information to be supplied**

Symbol	Title	Reference	Description
	Caution	ISO 7000-0434A	To indicate that caution is necessary when operating the device or control close to where the symbol is placed, or to indicate that the current situation needs operator awareness or operator action in order to avoid undesirable consequences.
	Manufacturer	ISO 7000-3082	To identify the manufacturer of a product.
	Operator's manual	ISO 7000-1641	To identify the location where the operator's manual is stored or to identify information that relates to the operating instructions. To indicate that the operating instructions should be considered when operating the device or control close to where the symbol is placed.
	Catalog number	ISO 7000-2493	To identify the manufacturer's catalog number, for example on a medical device or the corresponding packaging.
	Serial number	ISO 7000-2498	To identify the manufacturer's serial number, for example on a medical device or its packaging.
	Mass; weight	ISO 7000-1321B	To indicate mass. To identify a function related to mass.
	Locked.	ISO 7000-1655	To identify the locking control. To indicate that a control is locked. To indicate that the function cannot be changed or adjusted because its operation is locked. To identify the location of a lock.
	Unlocked.	ISO 7000-3305	To identify the control that effects an unlocking function. To indicate that the component or function is in its unlocked state.
	Fragile; handle with care	ISO 7000-0621	To indicate that the contents of the transport package are fragile and the package shall be handled with care.




**Table 1 ISO 7000 - Graphical symbols for use on equipment - Registered symbols and ISO 15223-1 - Medical devices - Symbols to be used with medical device labels, labeling and information to be supplied (continued)**

Symbol	Title	Reference	Description
	Keep away from rain	ISO 7000-0626	To indicate that the transport package shall be kept away from rain and in dry conditions.
	Humidity limitation	ISO 7000-2620	To indicate the acceptable upper and lower limits of relative humidity for transport and storage.
	Temperature limit	ISO 7000-0632	To indicate the maximum and minimum temperature limits at which the item shall be stored, transported or used.

**Table 2 ISO 7010 - Graphical symbols - Safety colors and safety signs - Registered safety signs**

Symbol	Title	Reference	Description
	General warning sign	ISO 7010-W001	To signify a general warning.
	Refer to instruction manual/booklet	ISO 7010-M002	To signify that the instruction manual/booklet must be read.
	No pushing	ISO 7010-P017	To prohibit pushing against an object.

**Table 3 Other Symbols**

Symbol	Description
	U.S. Federal law restricts this device to sale by or on the order of a licensed healthcare provider.
	Medical Device
	To indicate that the device may not be disposed of in landfill but must be recycled according to the European Waste Electrical and Electronic Equipment (WEEE) directive.

## 2.0 Warnings and Precautions

---



### **WARNING: Risk of Operator Injury and Damage to Equipment**

The Auxiliary Cart - Camera Cart system may be installed, maintained, repaired, and serviced only by qualified Synaptive Medical service representatives. There are no user-serviceable parts in the Auxiliary Cart - Camera Cart system.

No modification of the Auxiliary Cart - Camera Cart system is allowed.

The Auxiliary Cart - Camera Cart contains non-permanent fasteners that may become loose over time, potentially causing mounted components to become loose and fall. Inspect the Auxiliary Cart before each use to ensure that there are no loose components. If any loose components are discovered, do not use the cart and report the problem to Synaptive Customer Service.

Use of the Auxiliary Cart adjacent to or stacked with other equipment should be avoided because it could result in improper operation. If such use is necessary, observe the Auxiliary Cart and the other equipment to verify that they are operating normally.

Use only the approved power cord supplied with the Auxiliary Cart - Camera Cart. The use of non-approved power cords can result in damage to the Auxiliary Cart - Camera Cart system. The use of other accessories, transducers, and cables may result in increased electromagnetic emissions or decreased immunity of this equipment and may result in improper operation. If a cable becomes damaged, contact Synaptive customer service for assistance.

The cables connecting the Auxiliary Cart carts to each other and other equipment are a potential tripping hazard. When positioning the carts for a procedure, always ensure that there is sufficient cable length to allow the cables to reach the floor. Use caution when walking around the carts to avoid tripping over cables.

Before moving a cart, always ensure that all cart casters are unlocked. Push the carts using the cart handles only. Never push on surfaces marked with the Do Not Push symbol. Applying excessive force to the cart or its components may present a tipping hazard.

Do not move the Auxiliary Cart - Camera Cart with the tracking camera arm extended. Collapse the tracking camera arm and lock it in place before moving the cart. If the arm is not locked in place, it may extend unexpectedly and cause the Auxiliary Cart to tip over.

Always use caution around the tracking camera arm. If the internal gas spring fails, the camera may drop suddenly.

Use caution when moving the Auxiliary Cart - Camera Cart to prevent collisions with people or stationary objects such as equipment, doorways, or walls.

Do not roll the Auxiliary Cart - Camera Cart over cabling. Doing so may damage the cables and cause the Auxiliary Cart to become unusable. If a cart rolls over cabling, inspect the cable for damage. If a cart rolls over any object, inspect the castors for damage.

The Auxiliary Cart - Camera Cart contains a pressurized gas cylinder, which, although extremely unlikely, may suddenly rapidly decompress, potentially causing damage to equipment and injury to persons standing nearby.

---



**WARNING: Risk of Operator or Patient Injury Due to Laser Light Emission**

Do not look directly into the laser-emitting aperture on the tracking camera. The Class 2 laser module on the Position Sensor emits radiation that is visible and may be harmful to the human eye. Direct viewing of the laser diode emission at close range may cause eye damage.

Take precautions to ensure that people with restricted movement or reflexes (for example, patients undergoing medical procedures) do not look directly into the laser-emitting aperture. Patients undergoing medical procedures may not have normal adverse-effects reflexes (turning away eyes and/or head, closing eyes) due to pharmaceutical influences and/or mechanical restraints. The Class 2 laser module on the Position Sensor emits radiation that is visible and may be harmful to the human eye. Direct viewing of the laser diode emission at close range may cause eye damage.

Use of laser controls or adjustments or performance of laser-related procedures other than those specified herein may result in hazardous radiation exposure.



**WARNING: Risk of Electric Shock**

Use caution when handling the Auxiliary Cart - Camera Cart. If it develops a buildup of electric charge, anyone who touches the Auxiliary Cart may experience a mild shock.



**WARNING: Risk of Procedure Delay Due to Loss of Tracking**

Infrared sources in the operating room may interfere with tracking camera tracking. Remove any non-Synaptive sources of infrared signals from the operating room before performing a procedure using the tracking camera.

The tracking camera cannot track multiple instances of the same tool simultaneously. Use only one of each tool in the camera's field of view at a time.

Loss of power will result in loss of tracking capability. If power to the cart is cut off, restore the power or follow your site's established protocols to end the procedure.



**WARNING: Risk of Procedure Delay Due to Loss of Registration**

Always lock all casters on the Auxiliary Cart carts to prevent them from moving during the procedure.



**WARNING: Risk of Damage to Equipment**

Always verify that the cables connecting the Auxiliary Cart - Camera Cart to other Synaptive equipment are securely connected. Applying excessive force to the cables may cause them to become disconnected, potentially damaging the system.

When setting up equipment, avoid bending the cables excessively. Extreme bends may damage the cables and lead to loss of function.

Use only the cleaning agents described in this manual to clean the Auxiliary Cart - Camera Cart. Using other cleaning agents may damage the Auxiliary Cart.

## 3.0 Incident Reporting

Immediately report any serious incident that has occurred in relation to the use of this device to Synaptive Medical and, for EU customers, the competent authority of your Member State.

## 4.0 Intended Use Environment

The Auxiliary Cart - Camera Cart is intended for use in hospitals, clinics, and other medical institutions.

## 5.0 Synaptive Customer Service Information

For 24-hour access to clinical and technical support, contact Synaptive customer service.

Phone: 1-844-462-7246 (North America)

1-647-925-3435 (International)

Email: [service@synaptivemedical.com](mailto:service@synaptivemedical.com)

## 6.0 About the Auxiliary Cart - Camera Cart

The Camera Cart provides tool tracking for Synaptive systems like BrightMatter Guide and Modus V.

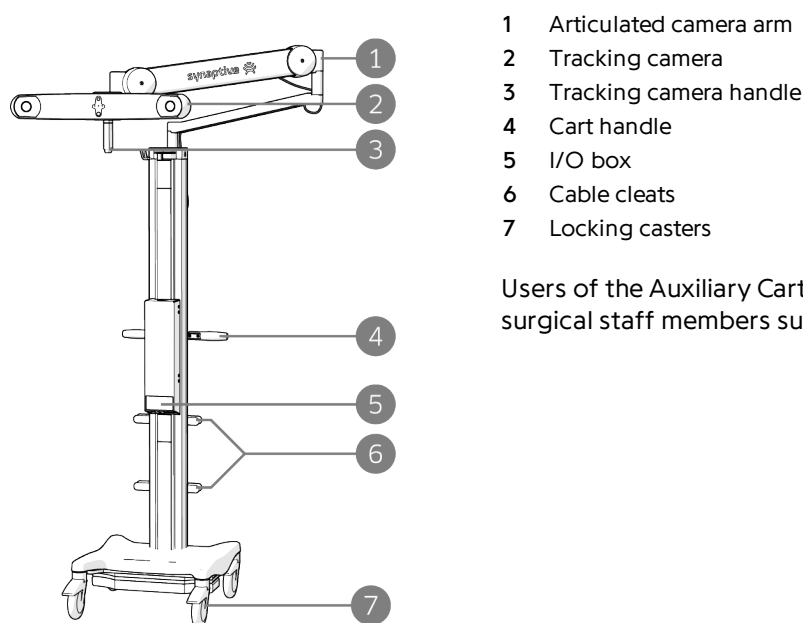


Figure 1 Camera Cart components

Users of the Auxiliary Cart - Camera Cart are surgeons and surgical staff members such as OR nurses.

## 7.0 About the Tracking Camera

The tracking camera works by emitting flashes of invisible (infrared) light that reflect off passive reflective markers on tracked instruments. The reflected light is captured by sensors on the tracking camera and is used to determine the position of the markers.

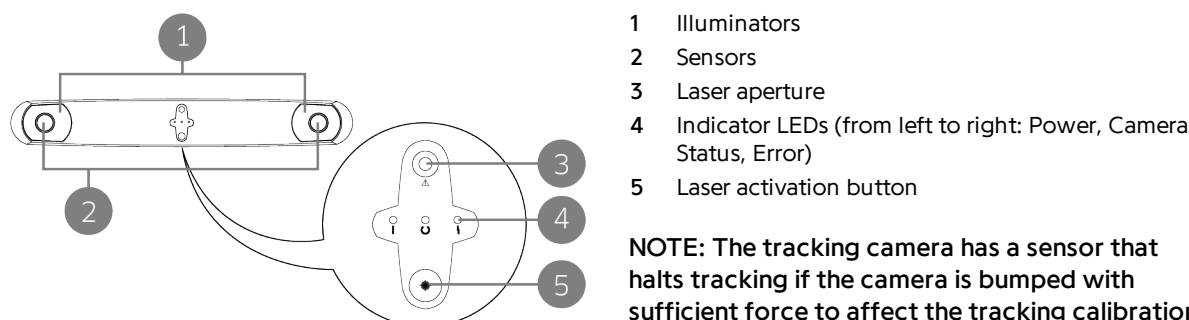


Figure 2 Tracking camera front view

- 1 Illuminators
- 2 Sensors
- 3 Laser aperture
- 4 Indicator LEDs (from left to right: Power, Camera Status, Error)
- 5 Laser activation button

**NOTE:** The tracking camera has a sensor that halts tracking if the camera is bumped with sufficient force to affect the tracking calibration. When the sensor is tripped, the camera Error LED flashes. If this occurs, you must contact Synaptive Service to re-calibrate the camera.

### 7.1 Using the Tracking Camera Positioning Laser

The tracking camera includes a positioning laser that indicates the center of the camera's tracking volume. Use this feature to orient the tracking camera towards the surgical site so all tools and the cranial reference are in the field of view. The laser beam is emitted from an aperture on the front of the tracking camera (item 4 in Figure 2 above).



#### **WARNING: Risk of Operator or Patient Injury Due to Laser Light Emission**

Do not look directly into the laser-emitting aperture on the tracking camera. The Class 2 laser module on the Position Sensor emits radiation that is visible and may be harmful to the human eye. Direct viewing of the laser diode emission at close range may cause eye damage.

Take precautions to ensure that people with restricted movement or reflexes (for example, patients undergoing medical procedures) do not look directly into the laser-emitting aperture. Patients undergoing medical procedures may not have normal adverse-effects reflexes (turning away eyes and/or head, closing eyes) due to pharmaceutical influences and/or mechanical restraints. The Class 2 laser module on the Position Sensor emits radiation that is visible and may be harmful to the human eye. Direct viewing of the laser diode emission at close range may cause eye damage.

Use of laser controls or adjustments or performance of laser-related procedures other than those specified herein may result in hazardous radiation exposure.

To use the positioning laser, press and hold the laser activation button on the front of the tracking camera (item 5 in Figure 2 above). The laser remains on only while the button is pressed.

## 7.2 Positioning Laser Battery

The laser can be activated whether the tracking camera is powered on or off. When the tracking camera is powered on, the laser draws power through the system from the mains supply. When the system is not powered on, the laser derives its power from an internal battery. If the laser battery needs to be replaced, contact Synaptive Service (for contact information, see 5.0 Synaptive Customer Service Information on page 8).

## 8.0 Using the Tracking Camera Arm

Use the tracking camera arm to position the tracking camera so that the patient reference and tracked surgical tools will be within the tracking camera's field of view throughout the surgical procedure.

The arm has three joints that rotate in the horizontal plane and two that rotate in the vertical plane allowing it to be moved into a wide range of positions.

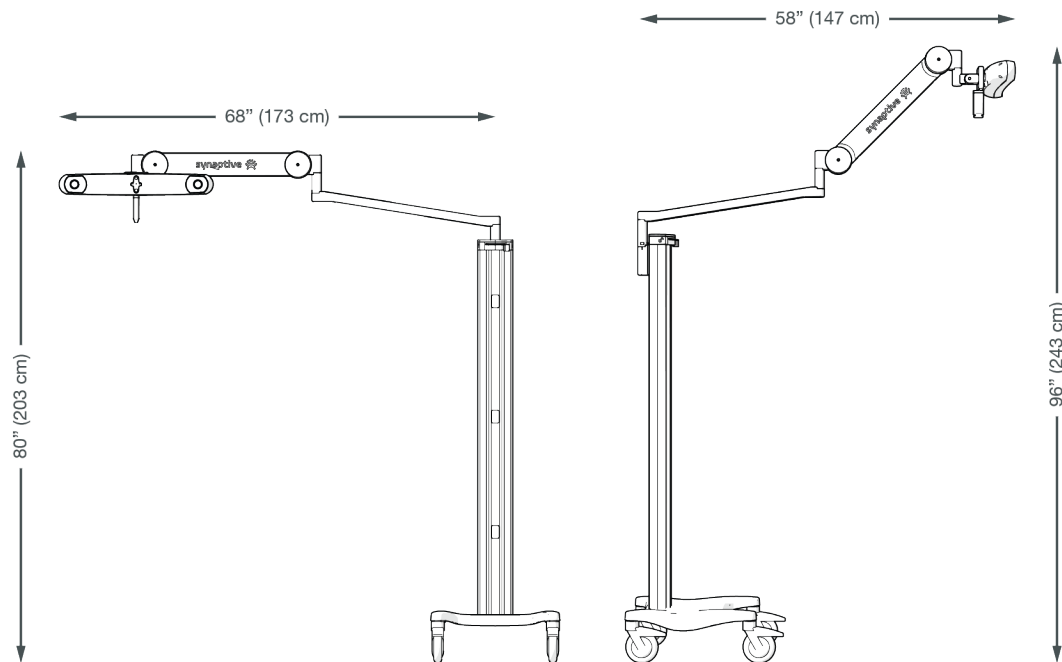


Figure 3 Reach of the tracking camera arm when fully extended horizontally and vertically



### WARNING: Risk of Operator Injury and Damage to Equipment

Do not move the Auxiliary Cart - Camera Cart with the tracking camera arm extended. Collapse the tracking camera arm and lock it in place before moving the cart. If the arm is not locked in place, it may extend unexpectedly and cause the Auxiliary Cart to tip over.

Always use caution around the tracking camera arm. If the internal gas spring fails, the camera may drop suddenly.

Use the handle on the tracking camera arm to adjust the arm position.

If the handle is out of reach when the tracking camera arm is extended to its highest position, it is acceptable to lower the arm by pulling on the upper arm bar instead of using the handle.

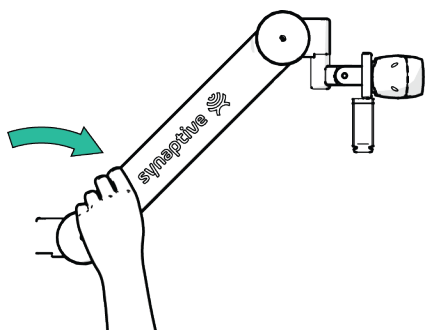


Figure 4 Lowering the arm when the handle is out of reach

The tracking camera arm has a lock feature that prevents the arm from moving when transporting or storing the cart.

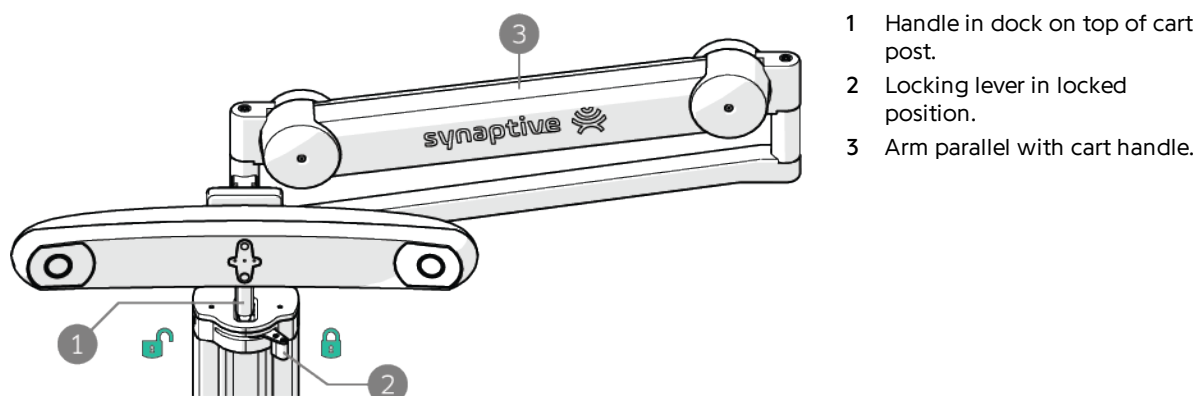


Figure 5 Arm in locked position

To lock the arm:

1. Position the arm so that the handle is in its dock on the top of the cart post.
2. Turn the locking lever to the locked position.
3. Rotate the arm to the right until it is parallel with the cart handle and the locking latch snaps into place. Note that there are alignment indicators on the arm and arm base to indicate when the arm is in the proper locked position.

To unlock the arm, turn the locking lever to the unlocked position.

## 9.0 Cart Connections



### **WARNING: Risk of Damage to Equipment**

Always verify that the cables connecting the Auxiliary Cart- Camera Cart to other Synaptive equipment are securely connected. Applying excessive force to the cables may cause them to become disconnected, potentially damaging the system.

When setting up equipment, avoid bending the cables excessively. Extreme bends may damage the cables and lead to loss of function.

Connect the tracking camera cable to the LEMO connector on the Auxiliary Cart - Camera Cart input/output box.



Figure 6 Cart inputs and outputs

## 10.0 Cleaning



### **WARNING: Risk of Damage to Equipment**

Use only the cleaning agents described in this manual to clean the Auxiliary Cart - Camera Cart. Using other cleaning agents may damage the Auxiliary Cart.

Cart surfaces may be cleaned with the following solutions:

- Water
- Mild Soap Solutions
- Hydrogen Peroxide Solution, 3%
- Iodine Solutions
- Bleach Solutions, 10%
- Isopropyl Alcohol Solutions, 70%, 91%
- Cavicide®

The cart surface finish will be permanently damaged by strong chemicals and solvents such as acetone and trichloroethylene. Steel wool or other abrasive material should never be used.

Never submerge or allow liquids to enter a cart or components on the cart. Doing so may irreparably damage the system. Wipe cleaning agents off surfaces immediately using a water-dampened cloth. Dry surfaces thoroughly after cleaning.

**CAUTION**

Synaptive Medical makes no claims regarding the efficacy of the listed chemicals or processes as a means for controlling infection. Consult your hospitals' infection control officer or epidemiologist.

## 11.0 Troubleshooting Problems

Table 4 Auxiliary Cart Problems and Possible Solutions

Problem	Possible Solutions
Tracked tools are not recognized by the tracking system.	<ul style="list-style-type: none"><li>• Ensure tracking camera has power.</li><li>• Ensure tracking spheres are clean and properly attached to the tool.</li><li>• Use the tracker calibration function in the BrightMatter Guide or Modus V software application to identify the positions of all tracked tools. Move the tracking camera so that all tools are inside the viewable volume.</li></ul>

## 12.0 Recommended Environmental Conditions

Operate, store, and transport the Auxiliary Cart system components only under the following conditions.

Table 5 Permissible Environmental Conditions

	Operating	Storage/Transport
Ambient temperature	10 °C–40 °C	-10 °C- 50 °C
Relative humidity (non-condensing)	30 %-75 %	10 %-90 %
Atmospheric Pressure	70 kPa–106 kPa	50 kPa–106 kPa

## 13.0 Disposal

Before disposing of any Synaptive product, contact Synaptive customer service or your supplier for further information.

## 14.0 System Classification and Specifications

**Classification:** Class II Equipment

**Mode of Operation:** Continuous Operation

**Degree of Protection Against Ingress of Water:** IPX0

## 15.0 Essential Performance

The camera shall transmit consistent data about the location of tracked tools.

## 16.0 Specifications

### 16.1 Cable Specifications

Table 6 Cable Specifications

Cable	Specifications
Camera cable	<ul style="list-style-type: none"><li>9 m shielded cable (14 x 28 AWG) with LEMO connector</li></ul>



#### WARNING

Use only the approved power cord supplied with the Auxiliary Cart - Camera Cart. The use of non-approved power cords can result in damage to the Auxiliary Cart - Camera Cart system. The use of other accessories, transducers, and cables may result in increased electromagnetic emissions or decreased immunity of this equipment and may result in improper operation. If a cable becomes damaged, contact Synaptive customer service for assistance.

### 16.2 Tracking Camera Laser Specifications and Standards

The positioning laser on the tracking camera is a Class 2 laser with a wavelength of 635 nm and a maximum output of 1 mW. The positioning laser conforms to the following standards:

- ANSI Z136.1 (2007)
- IEC 60825-1 (2007)
- FDA/CDRH 21 CFR 1040.10 and 1040.11 except for deviations pursuant to Laser Notice No. 50, dated June 24, 2007

## 17.0 Certifications

The Auxiliary Cart - Camera Cart is certified to the following standards:

- IEC 60601-1-2: 2014
- CAN/CSA C22.2 No. 60601-1: 2014-03
- ANSI/AAMI ES60601-1:2005/A1:2012-08
- CB SCHEME CERTIFICATION

All Auxiliary Cart Systems are designed and manufactured in an ISO:13485 registered facility that is routinely audited by medical device regulators under the Medical Device Single Audit Program (MDSAP).

## 18.0 Electromagnetic Environment Information

The Auxiliary Cart system requires special precautions regarding electromagnetic compatibility and must be installed and used according to the electromagnetic compatibility information described in the tables below.

Portable and mobile RF (radio frequency) communications equipment can affect the performance of the Auxiliary Cart system.

**Table 7 Electromagnetic Environment (Emissions)**

The Auxiliary Cart system is intended for use in the electromagnetic environment specified below. The customer or the user of the Auxiliary Cart system should assure that it is used in such an environment.

Emissions Test	Compliance	Electromagnetic Environment Guidance
RF emissions CISPR 11	Group 1	The Auxiliary Cart system uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.

Table 7 Electromagnetic Environment (Emissions) (continued)

Emissions Test	Compliance	Electromagnetic Environment Guidance
RF emissions CISPR 11	Class A	<p>The Auxiliary Cart system is suitable for use in all establishments other than domestic, and may be used in domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes, provided the following warning is heeded:</p> <p><b>Warning:</b> This equipment is intended for use by healthcare professionals only. This equipment may cause radio interference or may disrupt the operation of nearby equipment. It may be necessary to take mitigation measures, such as re-orienting or relocating the equipment or shielding the location.</p>
Harmonic emissions IEC 61000-3-2	Class A	
Voltage fluctuations/flicker emissions IEC 61000-3-3	Complies	

NOTE: The EMISSIONS characteristics of this equipment make it suitable for use in industrial areas and hospitals (CISPR 11 class A). If it is used in a residential environment (for which CISPR 11 class B is normally required) this equipment might not offer adequate protection to radio-frequency communication services. The user might need to take mitigation measures, such as relocating or re-orienting the equipment.

Table 8 Electromagnetic Environment (Immunity)

The Auxiliary Cart system is intended for use in the electromagnetic environment specified below. The customer or the user of the Auxiliary Cart system should assure that it is used in such an environment.

Immunity Test	IEC 60601 Test Level	Compliance Level	Electromagnetic Environment Guidance
Electrostatic discharge (ESD) IEC 61000-4-2	±8 kV contact ±15 kV air	±8 kV contact ±15 kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%.
Electrical fast transient/burst IEC 61000-4-4	±2 kV for power supply lines ±1 kV for input/output lines	±2 kV for power supply lines ±1 kV for input/output lines	Mains power quality should be that of a typical commercial or hospital environment.

Table 8 Electromagnetic Environment (Immunity) (continued)

Immunity Test	IEC 60601 Test Level	Compliance Level	Electromagnetic Environment Guidance
Surge IEC 61000-4-5	$\pm 0.5$ kV, $\pm 1$ kV line to line $\pm 0.5$ kV, $\pm 1$ kV, $\pm 2$ kV line to ground	$\pm 0.5$ kV, $\pm 1$ kV line to line $\pm 0.5$ kV, $\pm 1$ kV, $\pm 2$ kV line to ground	Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11 $U_T = 120$ Vac	0% $U_T$ (100% dip in $U_T$ ) for 0.5 cycle 0% $U_T$ (100% dip in $U_T$ ) for 1 cycle 70% $U_T$ (30% dip in $U_T$ ) for 25/30 cycles 0% $U_T$ (100% dip in $U_T$ ) for 5 sec	0% $U_T$ (100% dip in $U_T$ ) for 0.5 cycle 0% $U_T$ (100% dip in $U_T$ ) for 1 cycle 70% $U_T$ (30% dip in $U_T$ ) for 25/30 cycles 0% $U_T$ (100% dip in $U_T$ ) for 5 sec	Mains power quality should be that of a typical commercial or hospital environment. It is recommended that the Auxiliary Cart system be powered from an uninterruptible power supply or a battery.
Power frequency (50 Hz/60 Hz) magnetic field IEC 61000-4-8	30 A/m	30 A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.
NOTE $U_T$ is the a.c. mains voltage prior to application of the test level.			

**Table 9 Electromagnetic Environment (Conducted/Radiated)**

The Auxiliary Cart system is intended for use in the electromagnetic environment specified below. The customer or the user of the Auxiliary Cart system should assure that it is used in such an environment.

Immunity Test	IEC 60601 Test Level	Compliance Level	Electromagnetic Environment Guidance
Conducted RF IEC 61000-4-6	3 Vrms 150 kHz to 80 MHz  6 Vrms ISM/Amateur Radio bands inside 150 kHz to 80 MHz	3 Vrms 150 kHz to 80 MHz  6 Vrms ISM/Amateur Radio bands inside 150 kHz to 80 MHz	Portable and mobile RF communications equipment should be used no closer to any part of the Auxiliary Cart system, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter.  Recommended separation distance: $d = 1.2\sqrt{P}$
Radiated RF IEC 61000-4-3	3 V/m 80 MHz to 2,7 GHz	3 V/m 80 MHz to 2,7 GHz	$d = 1.2\sqrt{P}$ 80 MHz to 800 MHz $d = 2.3\sqrt{P}$ 800 MHz to 2.7 GHz  Where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in meters (m).  Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey <sup>a</sup> should be less than the compliance level in each frequency range <sup>b</sup> .

Note 1: At 80 MHz and 800 MHz, the higher frequency range applies.

Note 2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects, and people.

a) Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the Equipment is used exceeds the applicable RF compliance level above, the Auxiliary Cart system should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary such as re-orienting or relocating the Auxiliary Cart system.

b) Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.

**Table 10 Recommended Separation Distances Between Portable and Mobile RF Communications Equipment and the System**

The Auxiliary Cart system is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. Auxiliary Cart users can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the Auxiliary Cart system as recommended below, according to the maximum output power of the communications equipment.

Rated Maximum Output Power of Transmitter (W)	Separation Distance According to Frequency of Transmitter (m)		
	150 kHz - 80 MHz $d = 1.2\sqrt{P}$	80 MHz - 800 MHz $d = 1.2\sqrt{P}$	800 MHz - 2.7 GHz $d = 2.3\sqrt{P}$
0.01	0.12	0.12	0.24
0.1	0.38	0.38	0.73
1	1.2	1.2	2.3
10	3.8	3.8	7.3
100	12	12	23

For transmitters rated at a maximum output power not listed above, the recommended separation distance  $d$  in meters (m) can be estimated using the equation applicable to the frequency of the transmitter, where  $P$  is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

NOTE 1 At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

WARNING: Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the Auxiliary Cart system, including cables specified by the manufacturer. Otherwise, degradation of the performance of this equipment could result.

